



Proudly Owned and Operated in the USA

Searchable via: FreedomDiagnosticsTesting.com

Product	Slu-PP-332 & BAM15 300 mcg
Mass Identification	ERROR: Number of area count lines (2) does not match number of masses (1).

Certificate of Analysis

Accession Number	2512290158
Client	Pius Solutions Inc
Search Code	Pius2512290158




Received Date:	12/29/2025
Reported Date:	12/30/2025

Lot	N/A
Appearance	White Capsule

All Chemical Analysis was performed by HPLC with UV Detection Coupled with Mass Spectrometry

Mass Identification

Slu-PP-332/BAM15

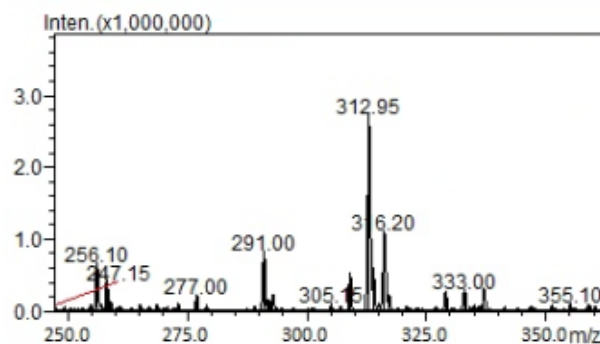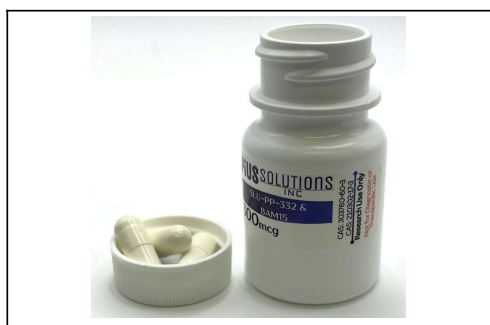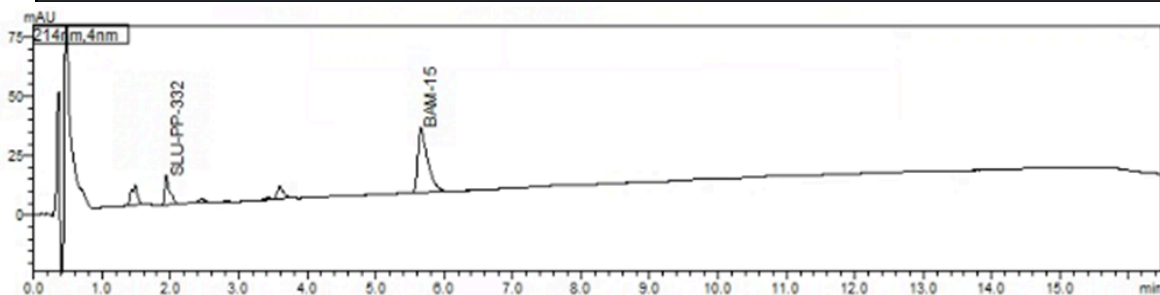

Stephen Schmidt

COA: 2512290158

Stephen Schmidt
Principal Chemist

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Searchable via: FreedomDiagnosticsTesting.com

Contact at: Admin@FreedomDiagnostics.net