



Client: Novaglo Research
Accession #: 2606100480
Search Code: Nova2606100480
Received: 06/10/2026
Reported: 06/12/2026
Lot: 50060626CJI


Sample Summary

Product:	CJC 1295/IPA (NO DAC)	Purity:	Vial 1: 99.98% Vial 2: 99.87% Vial 3: 99.90% Vial 4: 99.99% Vial 5: 99.79% Vial 6: 99.85% Vial 7: 99.96%
Identity:	Confirmed	Net Content:	Vial 1: Ipamorelin – 12.03 mg CJC-1295 – 11.18 mg Vial 2: Ipamorelin – 13.10 mg CJC-1295 – 10.92 mg Vial 3: Ipamorelin – 13.99 mg CJC-1295 – 11.45 mg Vial 4: Ipamorelin – 12.48 mg CJC-1295 – 11.72 mg Vial 5: Ipamorelin – 12.21 mg CJC-1295 – 10.65 mg Vial 6: Ipamorelin – 12.66 mg CJC-1295 – 10.39 mg Vial 7: Ipamorelin – 12.21 mg CJC-1295 – 11.98 mg
Appearance:	White Lyophilized Powder		
Endotoxin Threshold:	Pass		
Microbial Analysis (PCR):	Pass		
Fentanyl Screen	Negative		


Analytical Results

Test	Result	
Identity (LC-MS)	Ipamorelin/CJC-1295	
Purity (HPLC-UV)	99.91%	
Net Content Average	Ipamorelin - 12.67 mg CJC-1295 - 11.18 mg	
<i>Method: Endotoxin testing performed using Limulus Amebocyte Lysate assay in accordance with USP <85> under validated laboratory conditions.</i>		
Endotoxin Replicate 1:	Pass	Assay Sensitivity: ≤0.05 EU/mL
Endotoxin Replicate 2:	Pass	Assay Sensitivity: ≤0.05 EU/mL
<i>Method: Microbial detection performed using validated polymerase chain reaction (PCR)-based assay targeting common microbial contaminants.</i>		
Microbial Analysis (PCR)	No Detectable Microbial DNA	Pass
<i>Method: HPLC with UV detection coupled with mass spectrometry (LC-MS).</i>		

Chromatogram

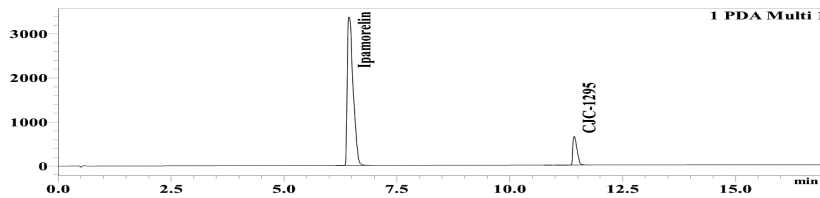

Mass Confirmation

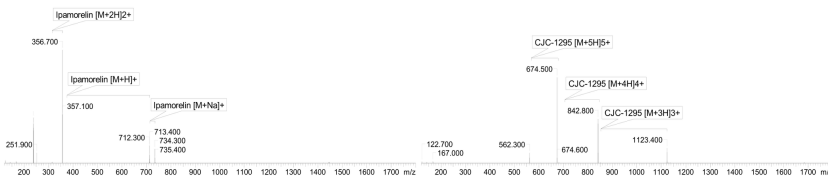

Alex Johnson
Principal Chemist

FreedomDiagnosticsTesting.com
Admin@FreedomDiagnostics.net

Proudly Owned and Operated in the US



The peptide purity analysis reported here was conducted using LC/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.